


Phase Noise $\mathcal{L}(f)$ in dBc/Hz

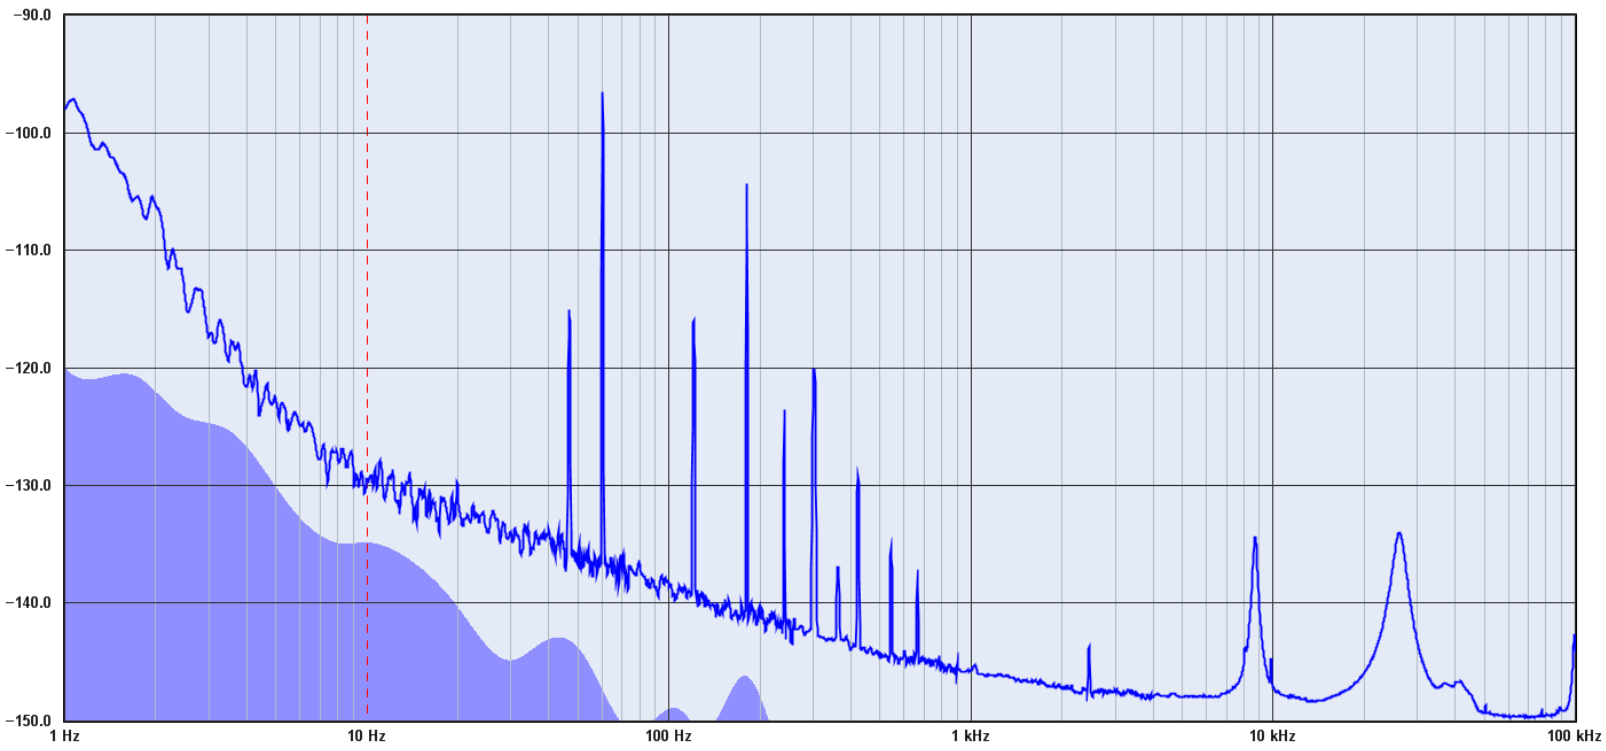

Trace	Notes	Input Freq	Sample Interval	dBc/Hz at 10 Hz	Duration	Acquired	Instrument
15 MHz vs ULN		15.000 MHz	0.010 s	-129.6	6m 13s	37330 pts	TimePod 5330A